

Figure 1

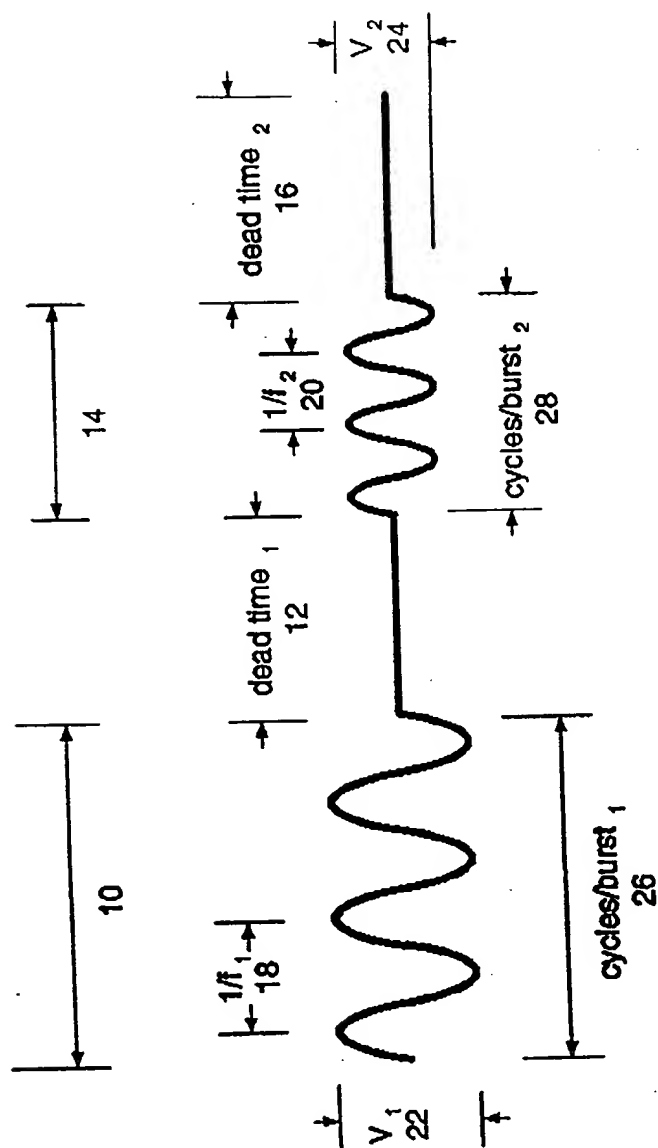


Figure 2

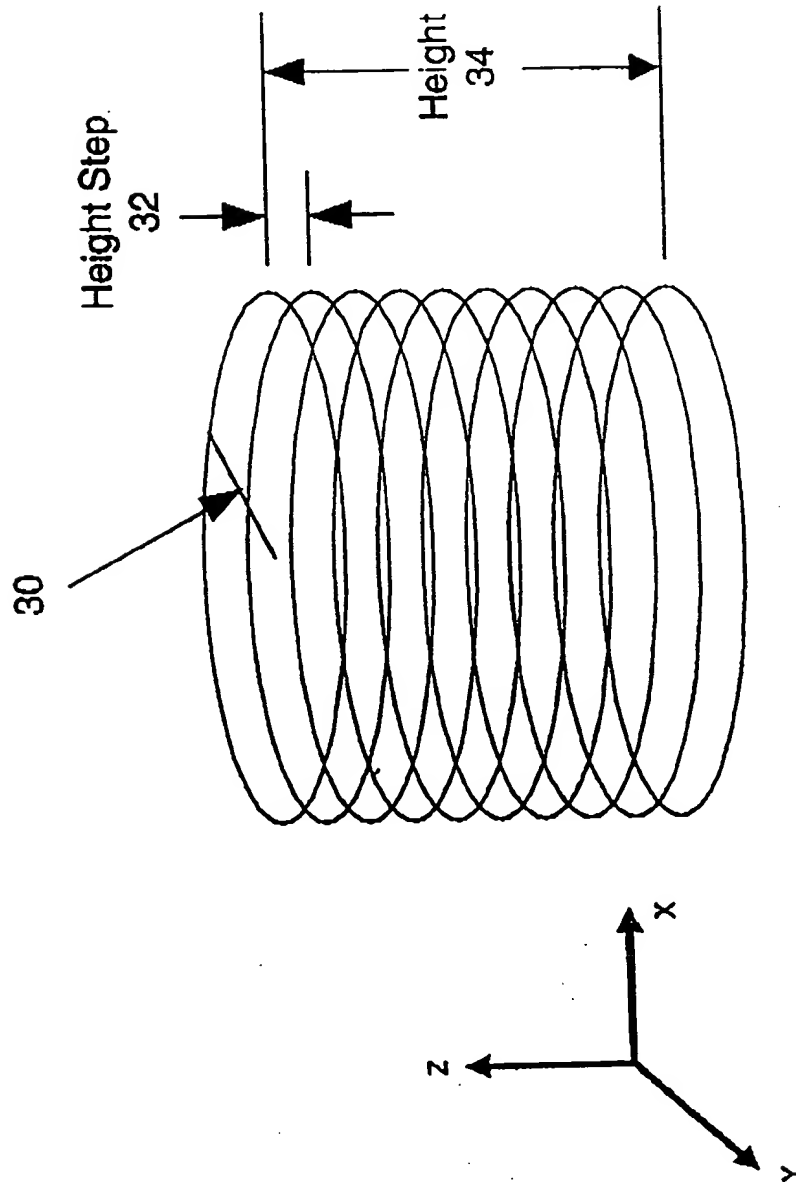


Figure 3

treatment
vessels




Fig. 4A




Fig. 4B




Fig. 4C

pre-treatment
assembly

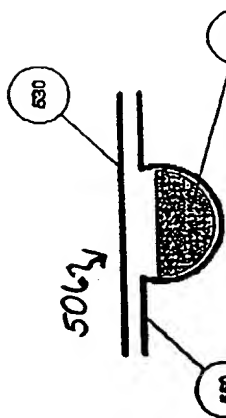


Fig. 5A

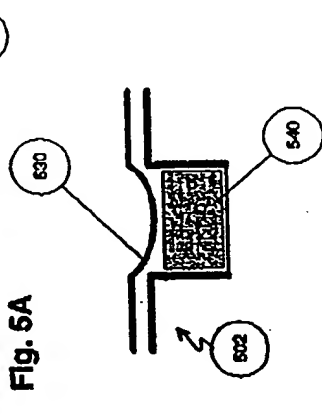


Fig. 5B

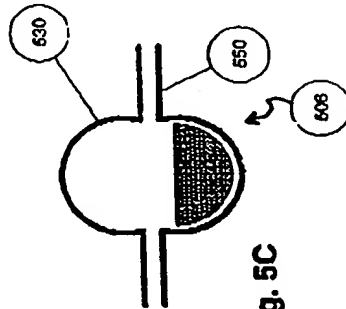


Fig. 5C

post-treatment
transfer

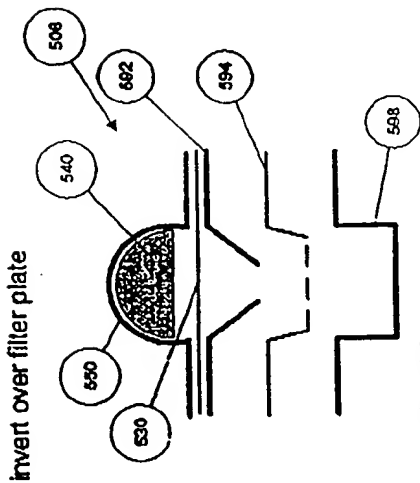


Fig. 6A

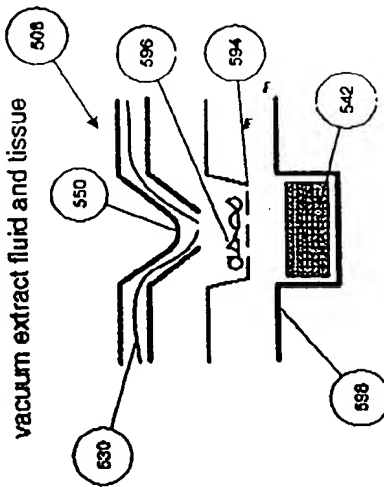


Fig. 6B

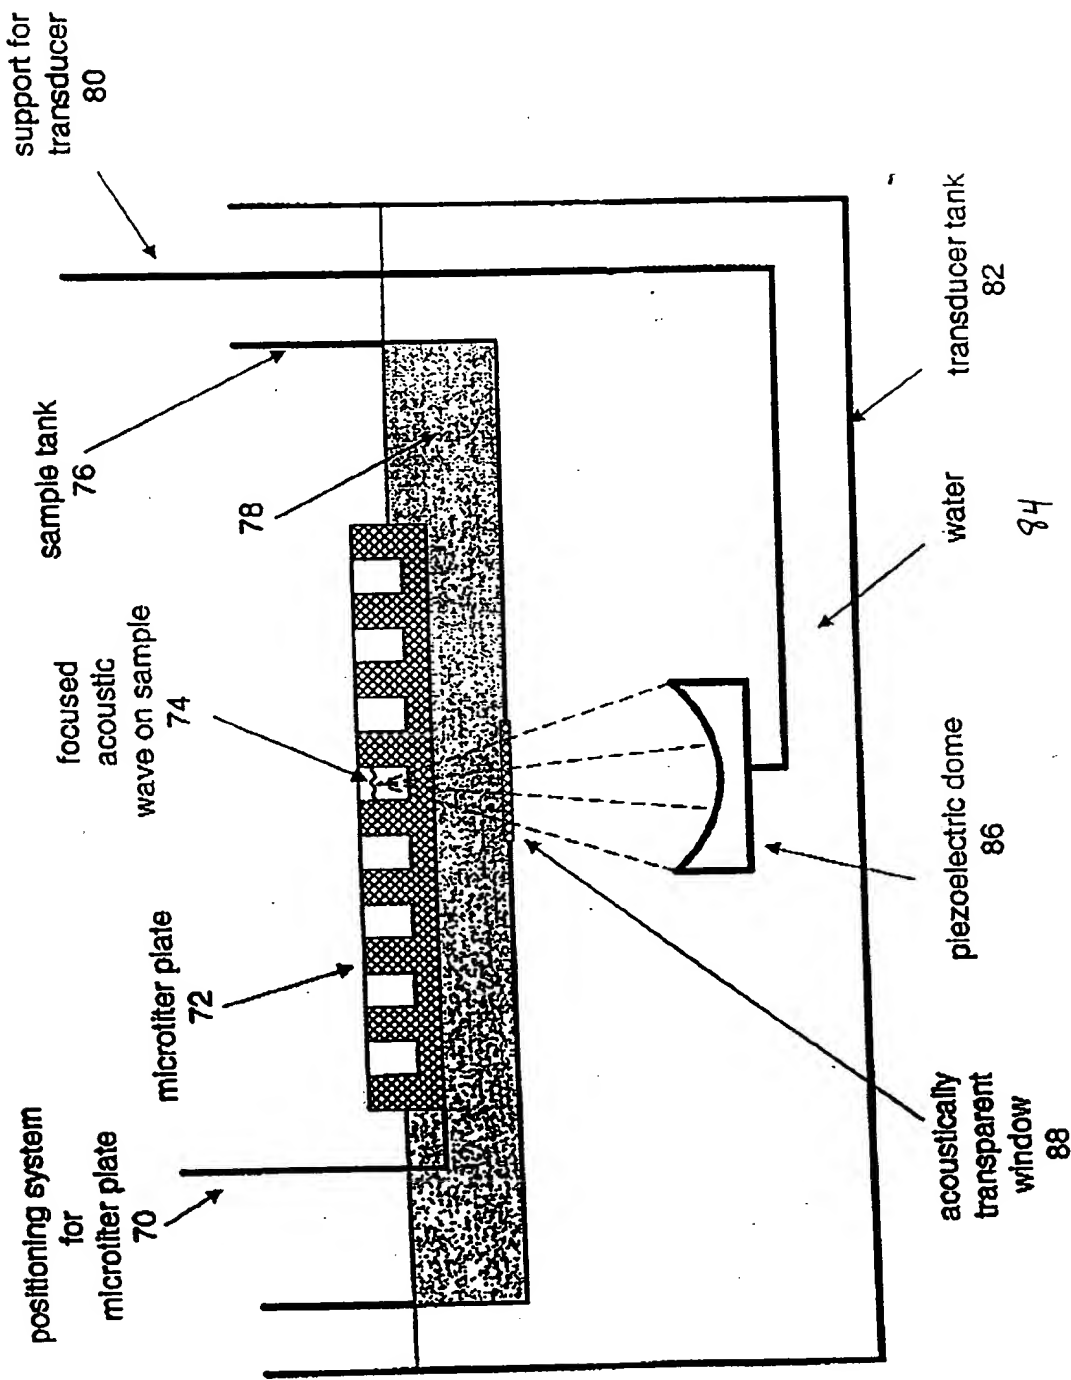


Figure 7


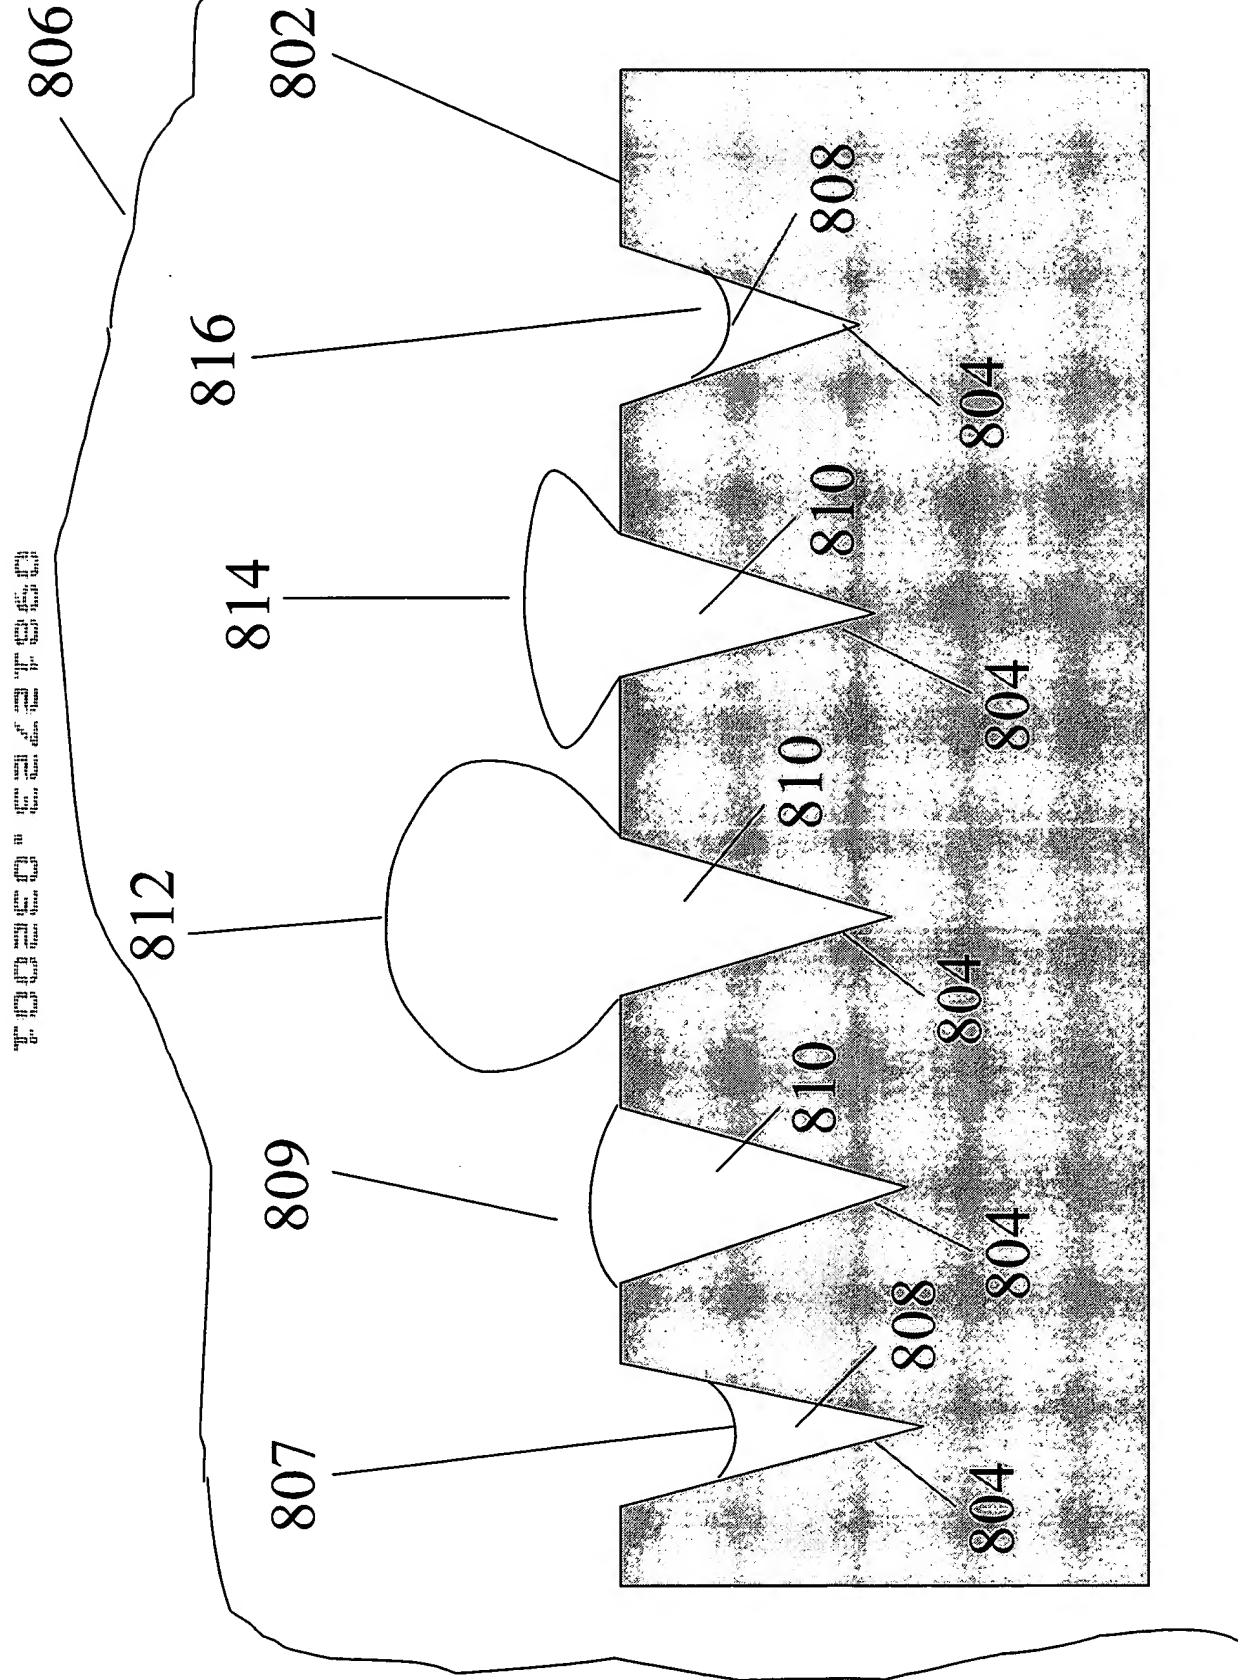


Figure 8
2046645

2046645

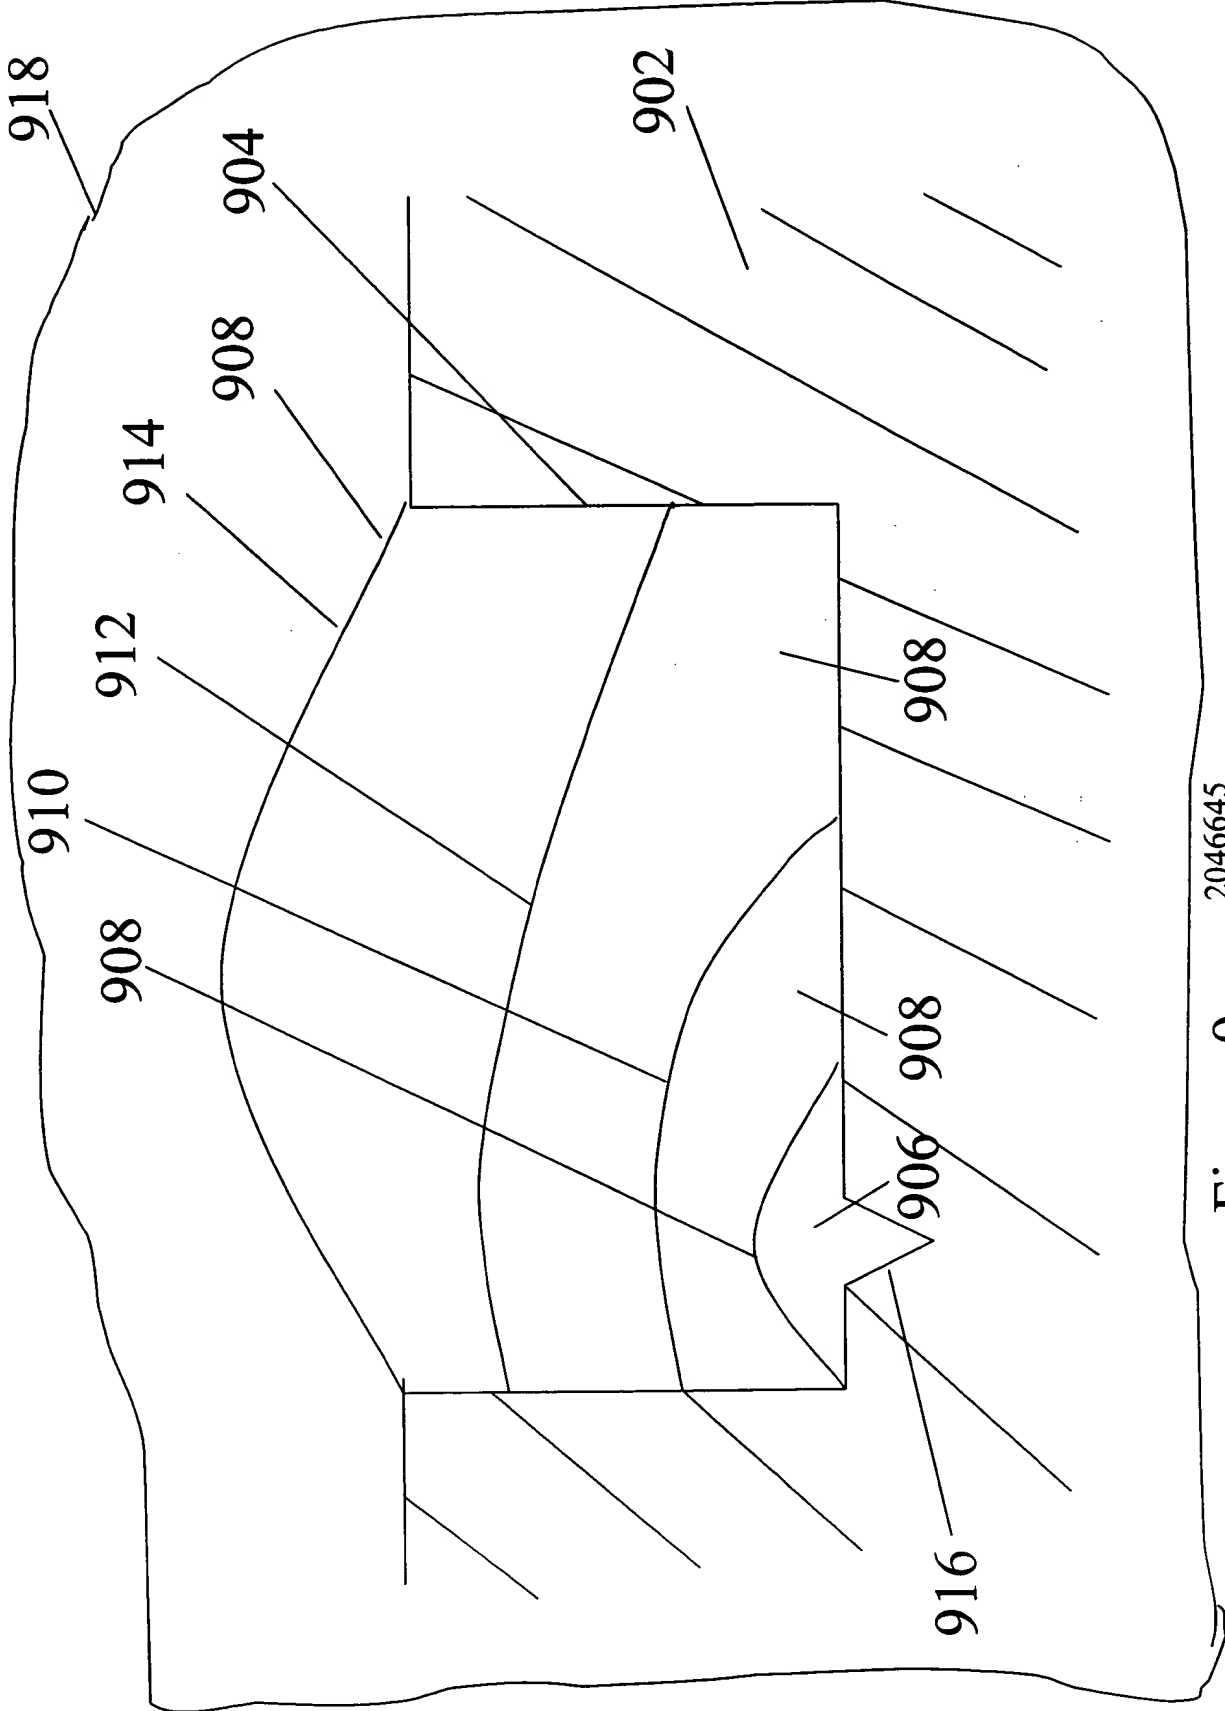

2046645

Figure 9

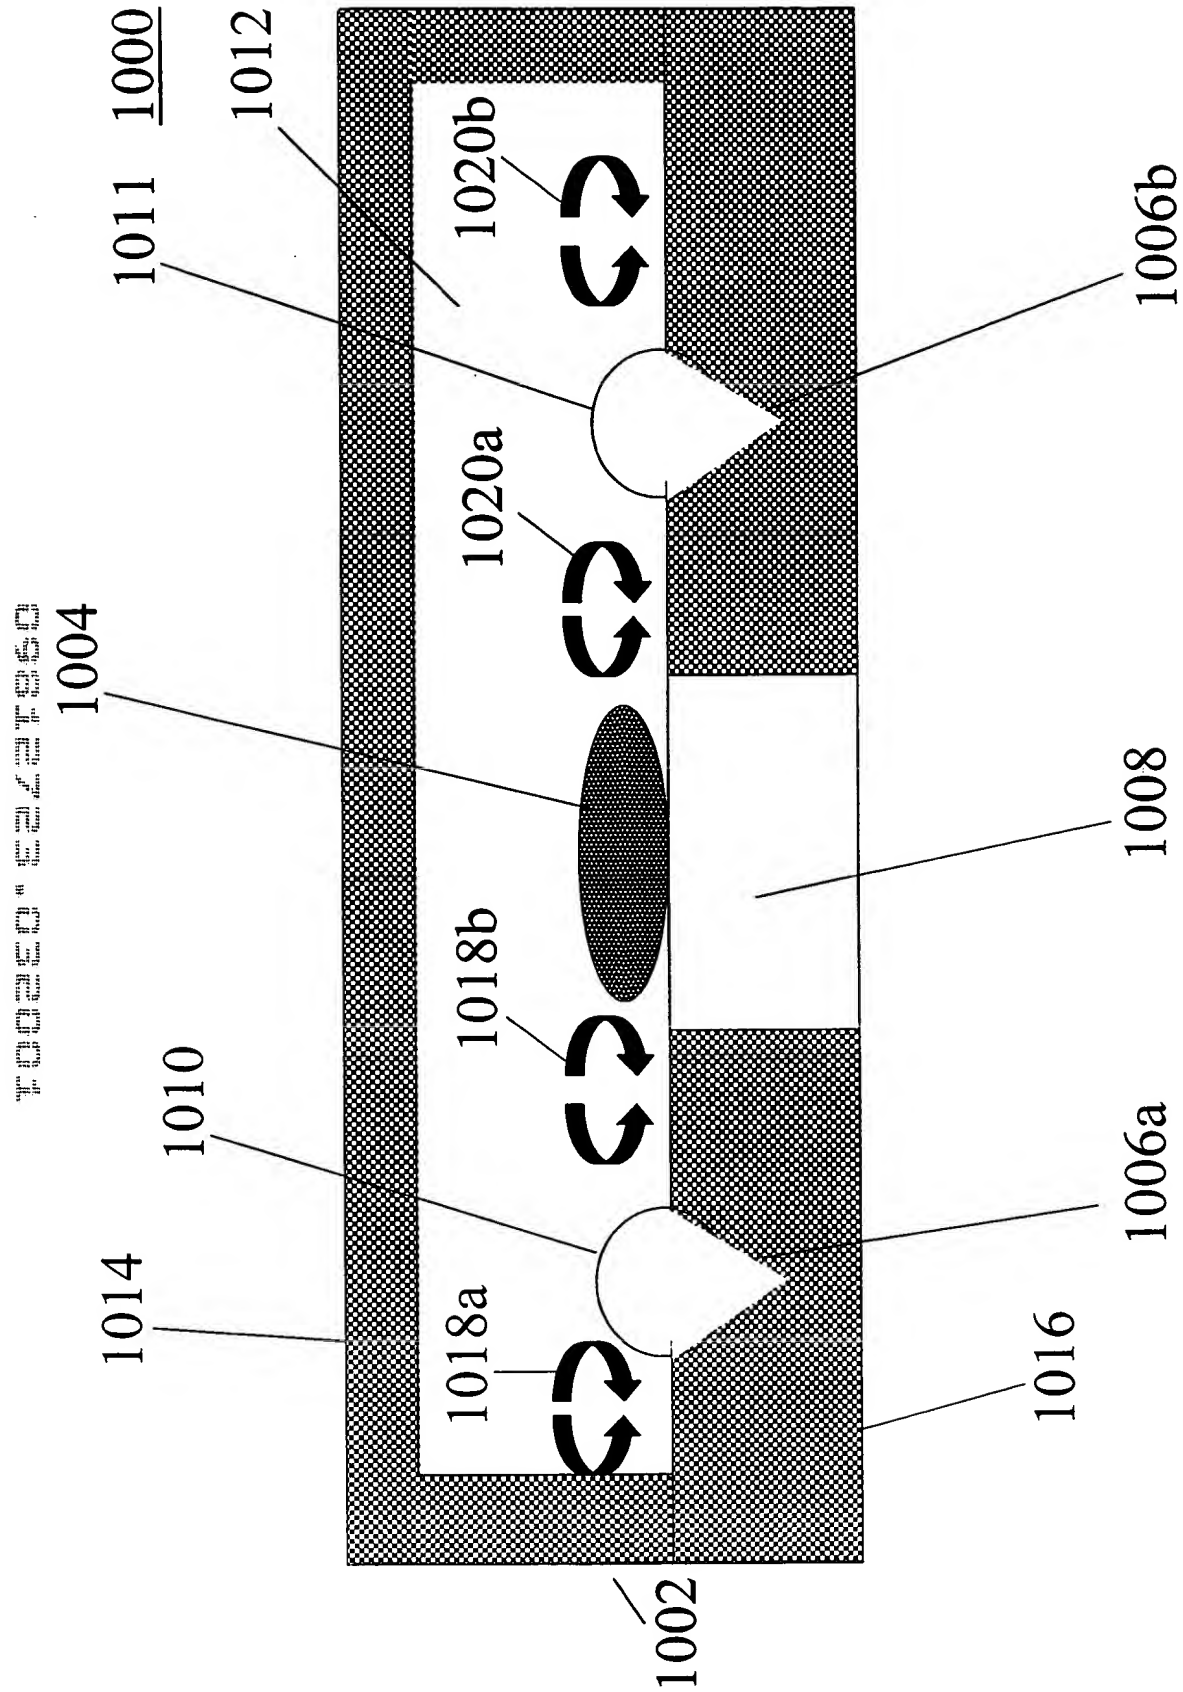


Figure 10
 2046645

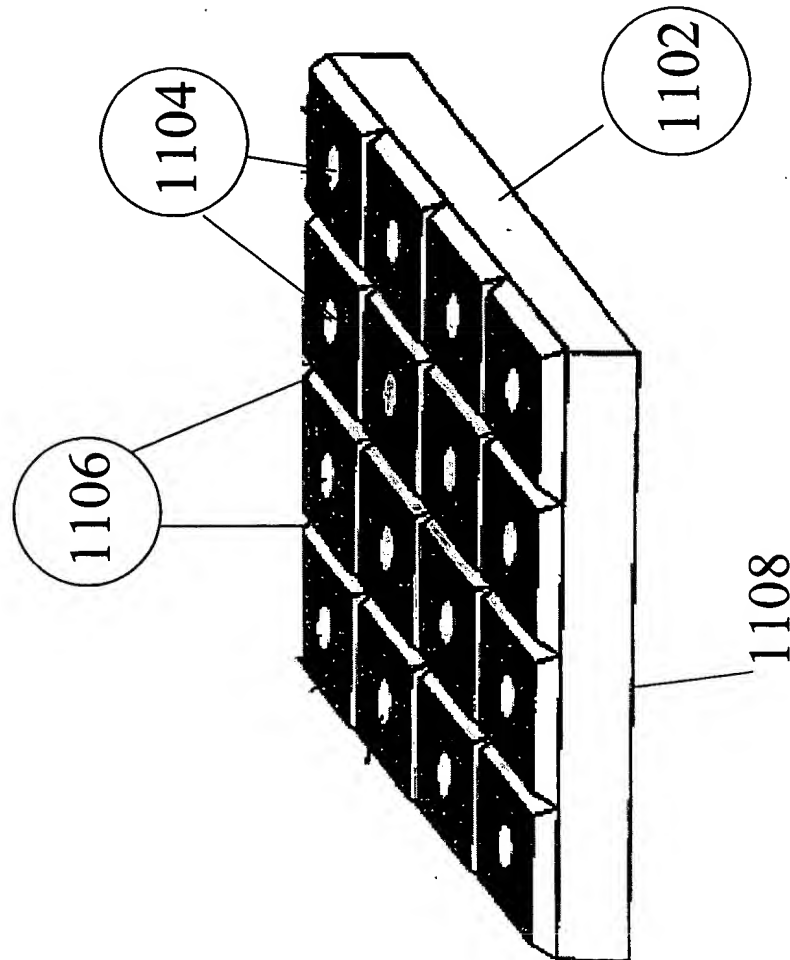


Figure 11

2046645

FIG. 11

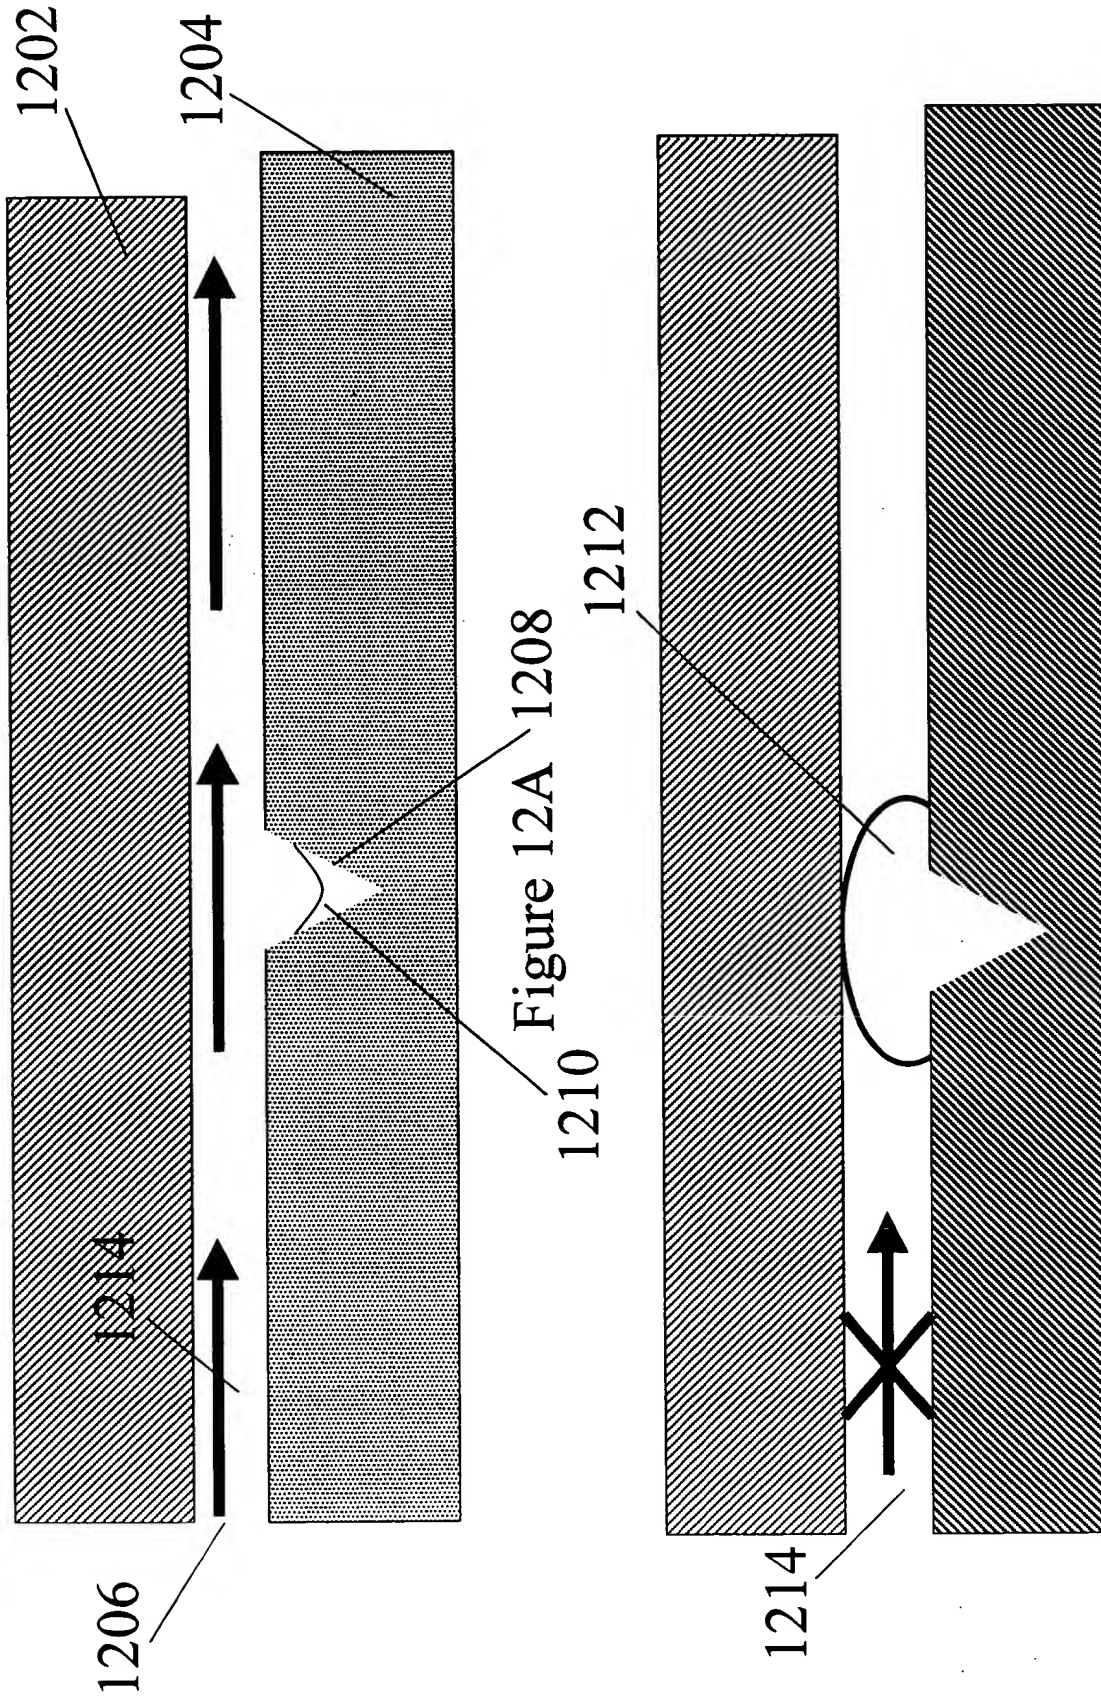


Figure 12B 2046645

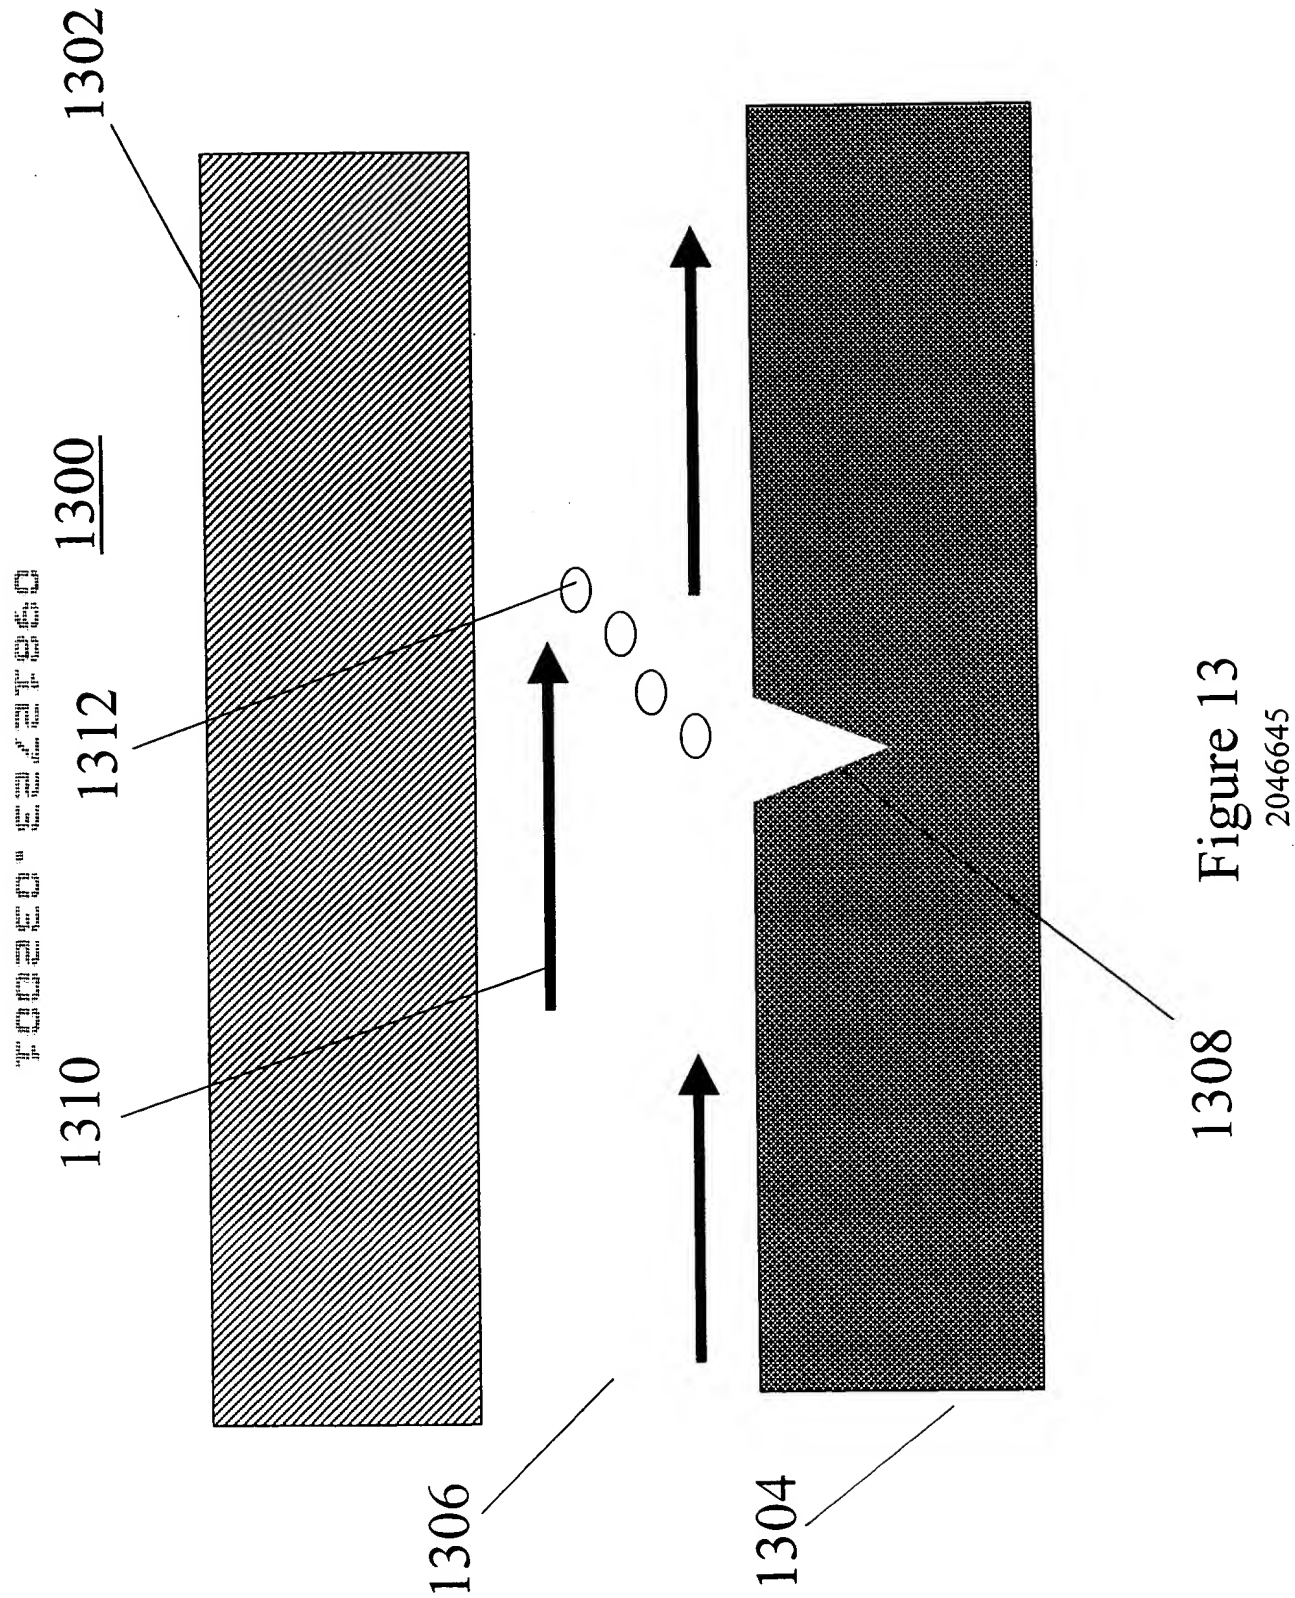


FIG. 14C

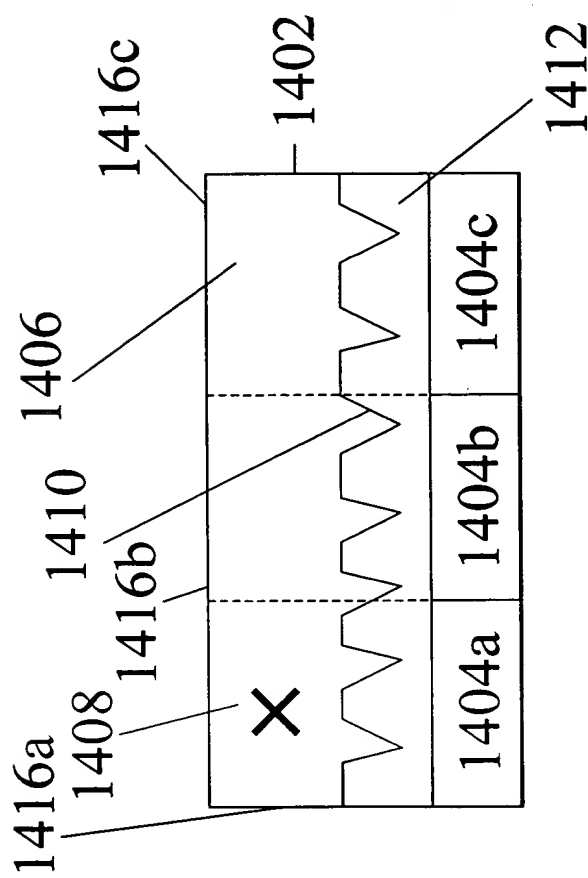


Figure 14A

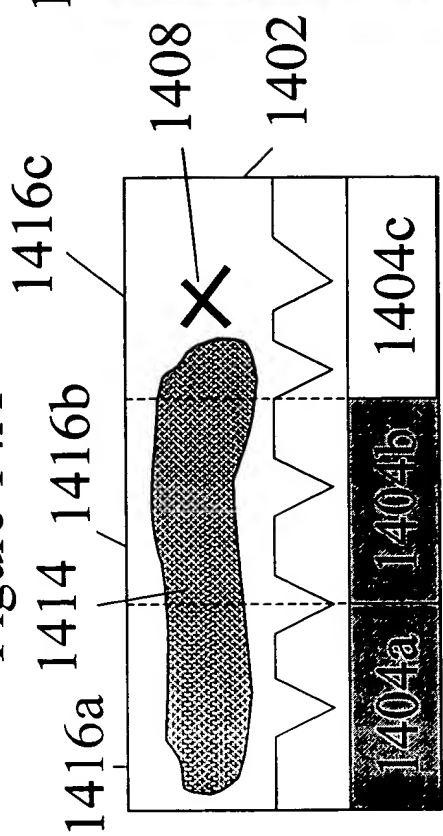


Figure 14B

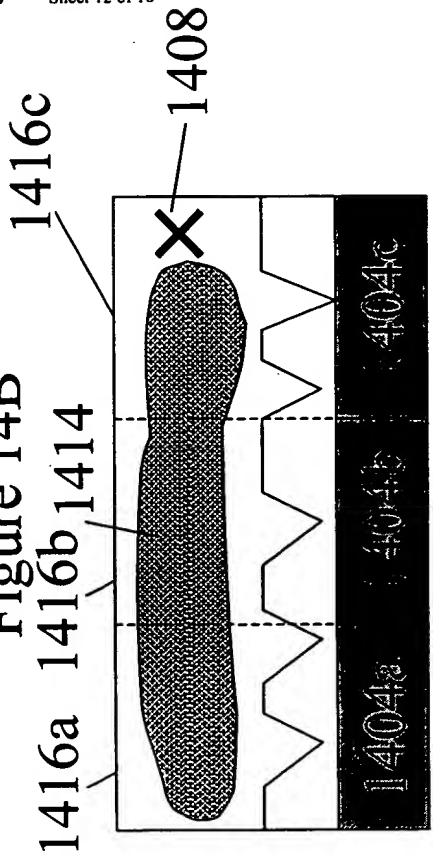


Figure 14C

Figure 14D



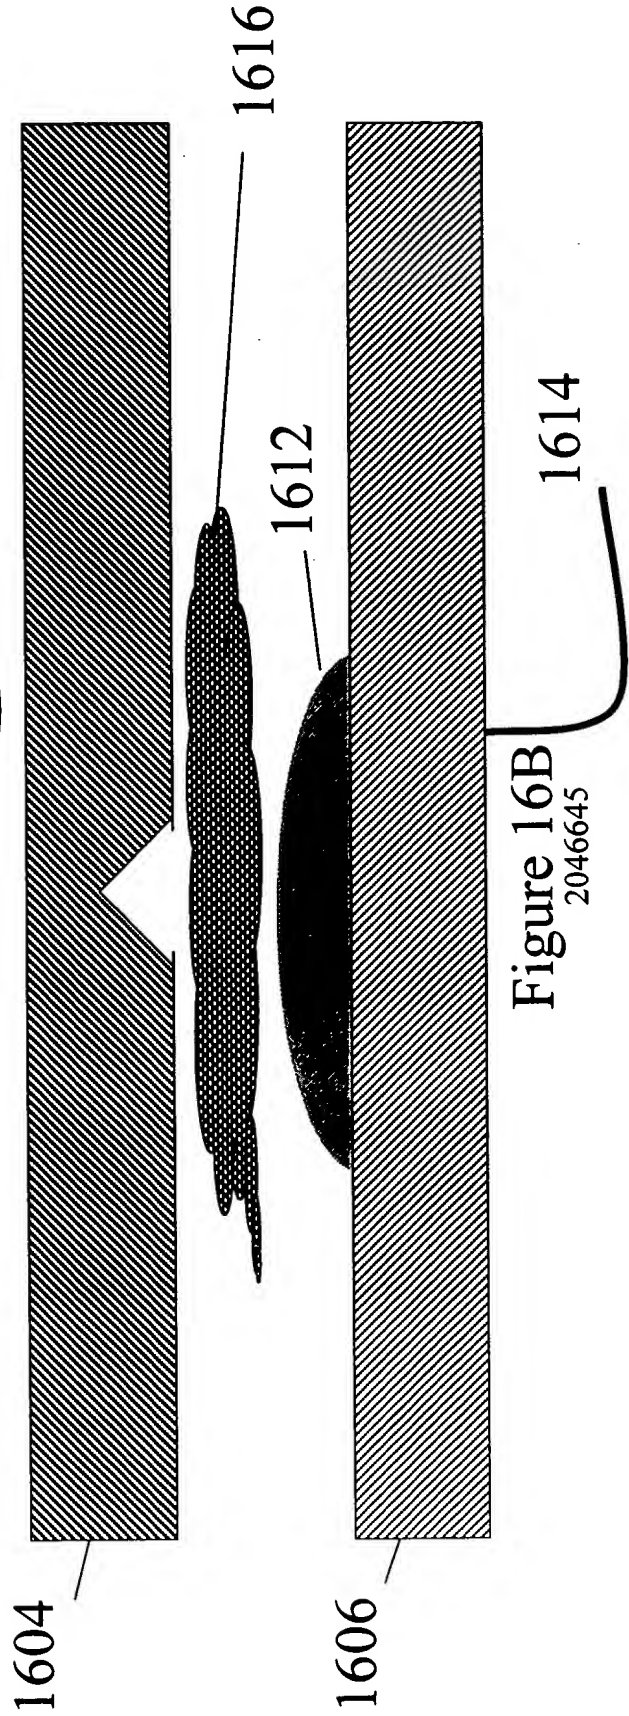
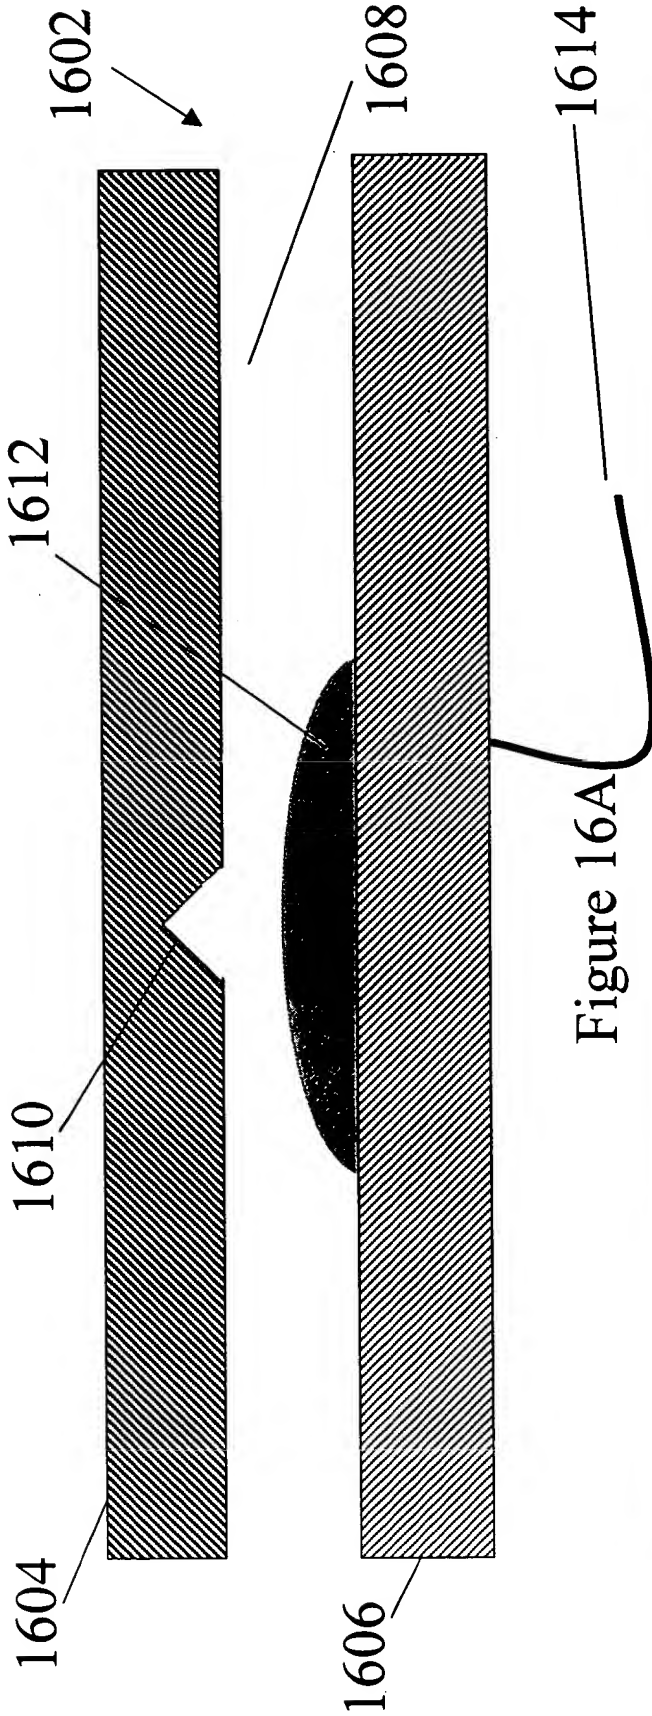


FIG. 17

1700

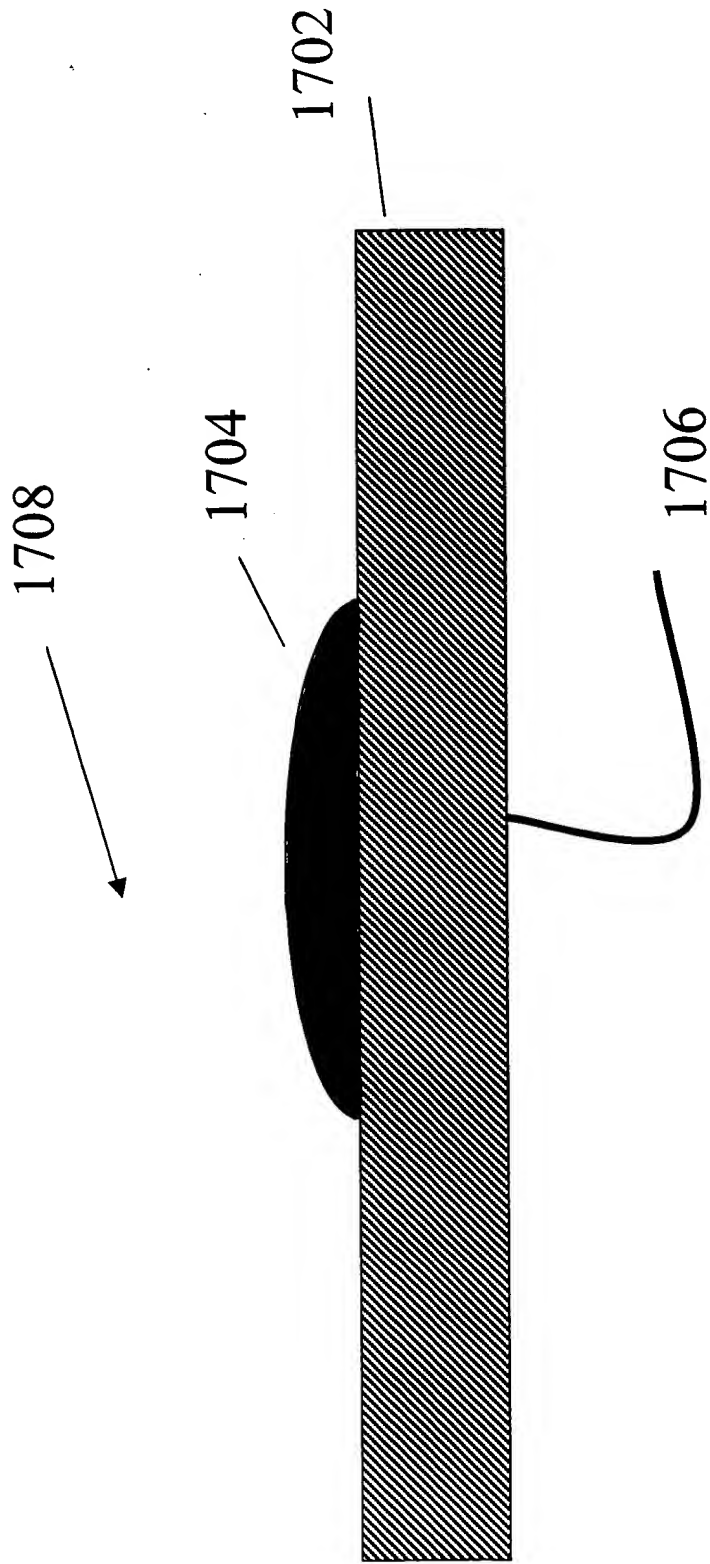


Figure 17

2046645

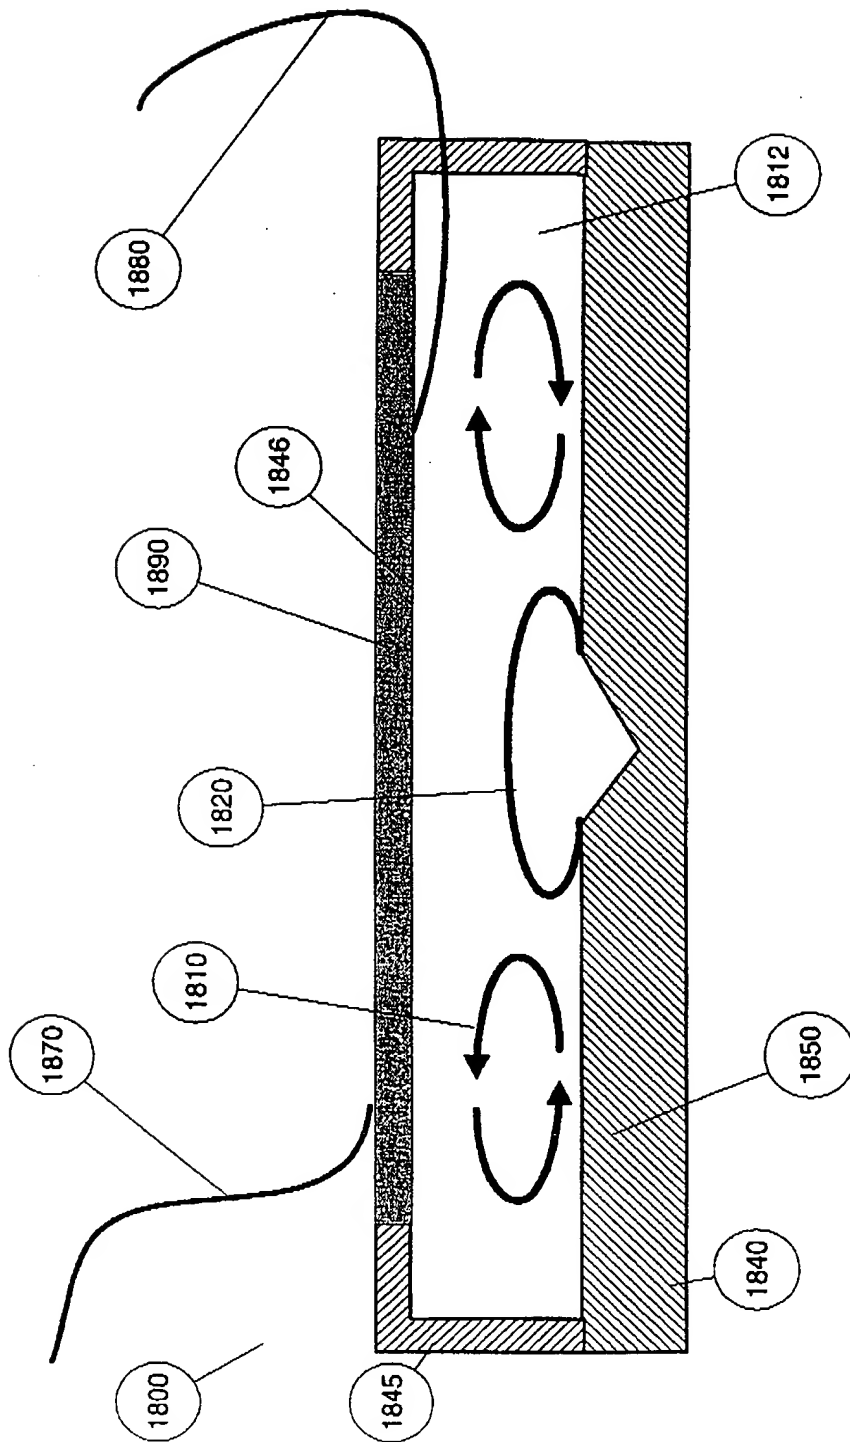


FIGURE EIGHTEEN